



CERTIFICATE OF ANALYSIS

SERAPREP

SP100 (1800-0020)

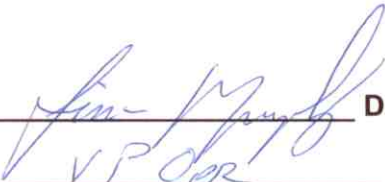
Product: SERAPREP
Part Number: SP100 (1800-0020)
Lot Number: 105020
Production Date: 24 MAY 2011
Expiration Date: 25 MAY 2012

Primary Application: Prepare serum and other native samples for amino acid analysis.

Acceptance Criteria:

- 1. pH = 1.04 ± 0.02 @ 25 °C (Y/N) y
- 2. Use threonine and serine peaks for evaluation. Serum sample peak times ± 30 seconds of calibration standard. (Y/N) y

Calibration Standard:
Physiological Fluid Calibration Standard, **PN** 011006P

Analysis Certified by:  Date: 02 JUN 2011
V.P. O'Connell
Title

ACCEPTED
PICKERING LABORATORIES, INC.
QUALITY ASSURANCE

Rev. 5, 04/08/2011